

General Parameters:


Program Name: Default.mo

Scan Parameters:

Scan Type: Standard Scan  
 Time/Date: 11:54:38 Thu Aug 27 2009  
 Data File Name: C:\DEKTA\DATA\Default\Default.001  
 Scan ID: 0  
 Stylus Type: Radius: 12.5 µm  
 Scan Length: 10000 µm  
 Resolution: 2.564 µm/sample  
 Stylus Force: 3 mg  
 Scan Length: 10000 µm  
 Samples: 3900  
 Duration: 13 sec  
 Meas Range: 2620 kÅ  
 Profile: Hills&Valleys

Display Parameters:

R. Cursor: 100 µm  
 R. Cursor Width: 0 µm  
 M. Cursor: 10000 µm  
 M. Cursor Width: 0 µm  
 Cursor ASH: -134432.7 Å  
 Vertical Distance: -134432.7 Å  
 Cursor Distance: 9900 µm  
 Display Range: Auto  
 Display Data Type: Raw

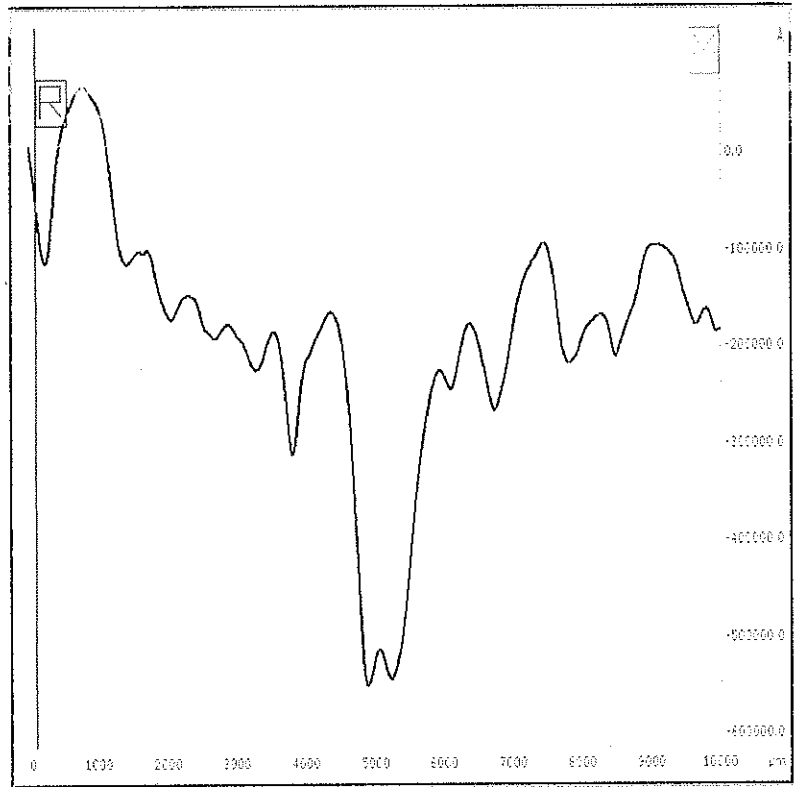

— Raw

Data Processing:

None

Analytical Functions:

Function Name	R. Cur Pos	R. Cur Width	M. Cur Pos	M. Cur Width	Result
~4	100 µm	0 µm	10000 µm	0 µm	83787.4A
Rv*	100 µm	0 µm	10000 µm	0 µm	121596.2A
Ro*	100 µm	0 µm	10000 µm	0 µm	-365368.1Å
Rt*	100 µm	0 µm	10000 µm	0 µm	210544.2Å
MaxRa*	100 µm	0 µm	10000 µm	0 µm	575912.2A
MaxDev*	100 µm	0 µm	10000 µm	0 µm	68017.5A
Skew*	100 µm	0 µm	10000 µm	0 µm	365368.1Å
RzDin*	100 µm	0 µm	10000 µm	0 µm	-1.2
					214209.4Å

Scan Data

General Parameters:


Program Name: Default.mp

Scan Parameters:

Scan Type: Standard Scan  
 Time/Date: 11:57:29 Thu Aug 27 2009  
 Data File Name: C:\DEKTA\DATA\Default\Default.001  
 Scan ID: 0  
 Stylus Type: Radius: 12.5  $\mu\text{m}$   
 Scan Length: 10000  $\mu\text{m}$   
 Resolution: 2.564  $\mu\text{m}/\text{sample}$   
 Stylus Force: 3 mg  
 Scan Length: 10000  $\mu\text{m}$   
 Samples: 3900  
 Duration: 13 sec  
 Meas Range: 2620 kÅ  
 Profile: Hills&Valleys

Display Parameters:

R. Cursor: 100  $\mu\text{m}$   
 R. Cursor Width: 0  $\mu\text{m}$   
 M. Cursor: 10000  $\mu\text{m}$   
 M. Cursor Width: 0  $\mu\text{m}$   
 Cursor ASH: -396178.8 Å  
 Vertical Distance: -396178.8 Å  
 Cursor Distance: 9900  $\mu\text{m}$   
 Display Range: Auto  
 Display Data Type: Raw

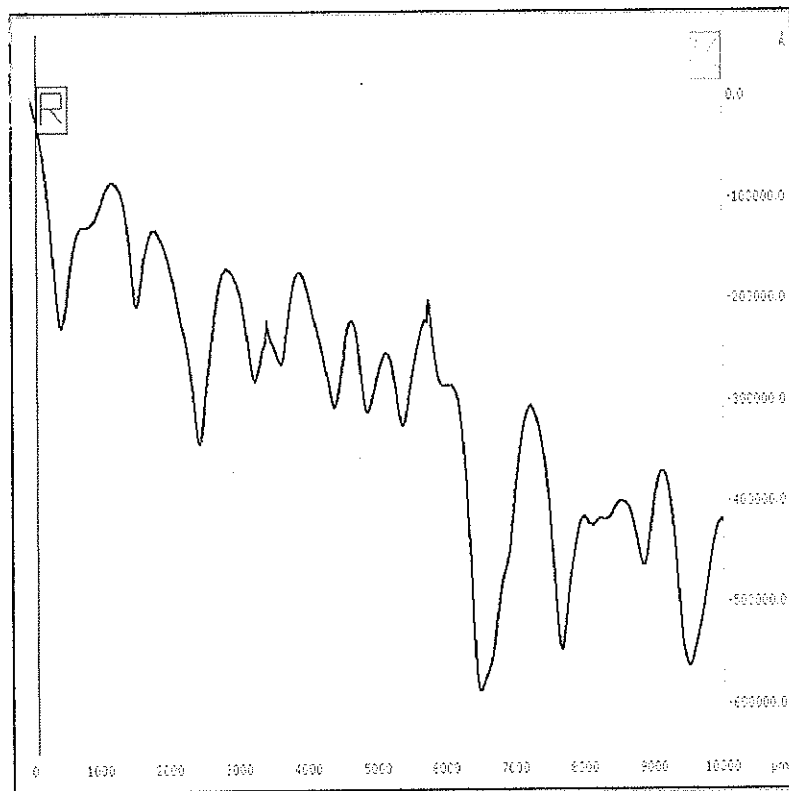

— Raw

Data Processing:

None

Analytical Functions:

Function Name	R. Cur Pos	R. Cur Width	M. Cur Pos	M. Cur Width	Result
Ra*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	49485.1 Å
Rq*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	65890.1 Å
Rv*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	-228421.5 Å
Rp*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	127823.4 Å
Rt*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	356244.9 Å
MaxRa*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	78878.1 Å
MaxDev*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	228421.5 Å
Skew*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	-1.2
RzDin*	100 $\mu\text{m}$	0 $\mu\text{m}$	10000 $\mu\text{m}$	0 $\mu\text{m}$	212263.1 Å